

AD-A164 366 RADIATION MEASUREMENTS FOR UCSB FEL(U) CALIFORNIA UNIV

RADIATION MEASUREMENTS FOR UCSB FEL(U) CALIFORNIA UNIV
CONF-8808020 QUANTUM INST 1-205004-2 57 21 1988

1/1

RADIATION MEASUREMENTS FOR UCSB FELLOWS, CALIFORNIA
SANTA BARBARA QUANTUM INST. I BOSCOLO ET AL. 1983

QIFEL-021/83 N00014-80-C-0308

UNCLASSIFIED


F/G 20/5

NL

END

FILMED
15 Feb

6716

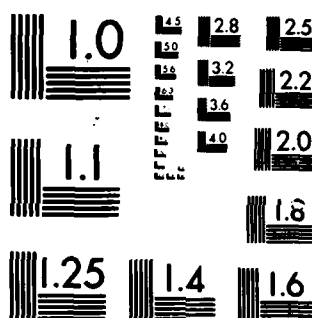

MICROCOPY RESOLUTION TEST CHART
NATIONAL BUREAU OF STANDARDS-1963-A

Unclassified/Unlimited

SECURITY CLASSIFICATION OF THIS PAGE (When Data Entered)

12

REPORT DOCUMENTATION PAGE

READ INSTRUCTIONS
BEFORE COMPLETING FORM

1. REPORT NUMBER No. 21	2. GOVT ACCESSION NO.	3. RECIPIENT'S CATALOG NUMBER
4. TITLE (and Subtitle) Radiation Measurements for UCSB FEL		5. TYPE OF REPORT & PERIOD COVERED Technical Report 10/01/82 - 09/30/83
		6. PERFORMING ORG. REPORT NUMBER
7. AUTHOR(s) Ilario Boscolo and Luis R. Elias		8. CONTRACT OR GRANT NUMBER(s) N00014-80-C-0308
9. PERFORMING ORGANIZATION NAME AND ADDRESS University of California Quantum Institute Santa Barbara, CA 93106		10. PROGRAM ELEMENT, PROJECT, TASK AREA & WORK UNIT NUMBERS 61153N; RR011-07-06; NR603-001
11. CONTROLLING OFFICE NAME AND ADDRESS ONR 1030 E. Green St. Pasadena, CA 91106		12. REPORT DATE 1983
		13. NUMBER OF PAGES
14. MONITORING AGENCY NAME & ADDRESS (if different from Controlling Office)		15. SECURITY CLASS. (of this report) Unclassified/Unlimited
		15a. DECLASSIFICATION/DOWNGRADING SCHEDULE

16. DISTRIBUTION STATEMENT (of this Report)

Approved for public release; distribution.

DTIC
ELECTE
FEB 18 1986
S D

17. DISTRIBUTION STATEMENT (of the abstract entered in Block 20, if different from report)

18. SUPPLEMENTARY NOTES

Proceedings of the International Conference of Lasers '82, 159, 1983.

19. KEY WORDS (Continue on reverse side if necessary and identify by block number)

Radiation, FEL

20. ABSTRACT (Continue on reverse side if necessary and identify by block number)

A calibrated He-cooled Ge-bolometer will be used to measure 2nW average spontaneous power at 380 um wavelength; the spectral analysis will use a Fabry-Perot. The more powerful laser output will be analyzed by a heterodyne spectrometer.

DD FORM 1 JAN 73 1473

86 2 18 040
Unclassified/Unlimited
SECURITY CLASSIFICATION OF THIS PAGE (When Data Entered)

AD-A164 366

DTIC FILE COPY

RADIATION MEASUREMENTS FOR UCSB-FEL

I. Boscolo, L. Elias, J. Ramian

QIFEL021/83

RADIATION MEASUREMENTS FOR UCSB-FEL

I. Boscolo,* L. Elias, J. Ramian
University of California, Santa Barbara

Abstract

A calibrated He-cooled Ge-bolometer will be used to measure 2 nW average spontaneous power at 380 μ m wavelength; the spectral analysis will use a Fabry-Perot. The more powerful laser output will be analyzed by a heterodyne spectrometer.

Introduction

The machine being constructed at the University of California at Santa Barbara will operate in two stages: in the first it will produce high power of infrared radiation and in the second this radiation will be efficiently up-converted (through the stimulated Compton scattering) into the optical region up to the UV region⁽¹⁾. In this paper we are concerned with the measurement of the FIR radiation, that is, both the spontaneous and the laser radiation at 380 μ m.

The very small power of spontaneous radiation ($\langle P_{\text{spont}} \rangle = 1 \text{ nW}$) requires a careful optics design. In contrast, the high power of the stimulated emission ($P_{\text{peak}} = 5 \div 15 \text{ kW}$) and the long length of the pulse allow a relatively softer hardware.

For ease of reference the UCSB-FEL parameters are listed below.

Characteristics of the spontaneous power

The spontaneous power is given by⁽²⁾

$$P_{\text{spont}} = \frac{I}{e} h \omega \cdot n$$

$$n = \pi \alpha N \left(\frac{\gamma \theta K}{1+K^2} \right)^2 \quad (1)$$

where n is the number of photons diffused by one electron in the trip, α the fine structure constant and θ is the angle of scattering. Substituting in (1) the parameters of table 1, we get

$$P_{\text{spont}} = 0.6 \text{ mW} \quad (2)$$

Since the response time of the power detectors is long, we have to measure the average power. This last, being the repetition rate 10 Hz, is

$$\langle P_{\text{spont}} \rangle = 0.9 \mu \text{W} \quad (3)$$

The power will be emitted into the solid angle

$$\Delta \Omega = \frac{\pi}{\gamma^2} \quad (4)$$

Table 1. UCSB-FEL parameters

Electron beam	Plane wiggler	Radiation and cavity
$E = 3 \text{ MeV}$	$L = 5.75 \text{ m}$	$L_{\text{cavity}} = 7.1 \text{ m}$
$\gamma = 6.38$	$\lambda_w = 3.6 \text{ cm}$	$\lambda_{\text{laser}} = 380 \mu \text{m}$
$I = 2 \text{ A}$	$N = 160$	$P_{\text{peak}} = 0.6 \text{ mW}$
$r = 3 \text{ mm}$	$B_0 = 670 \text{ Gauss}$	$\langle P_{\text{spont}} \rangle = 0.9 \text{ nW}$
$T = 150 \mu \text{sec}$	$K = 0.16$	$P_{\text{peak}} = 5 \div 15 \text{ kW}$
$f = 10 \text{ Hz}$		$\Delta \nu_{\text{spont}} = 3 \text{ GHz}$
$\frac{\Delta \gamma}{\gamma} \sim 10^{-5}$		$\Delta \theta = 2 \cdot 10^{-2} \text{ sterad}$

Permanent address Physics Department University of Lecce, Italy.



Codes	
Dist	Avail and/or Special
A-1	

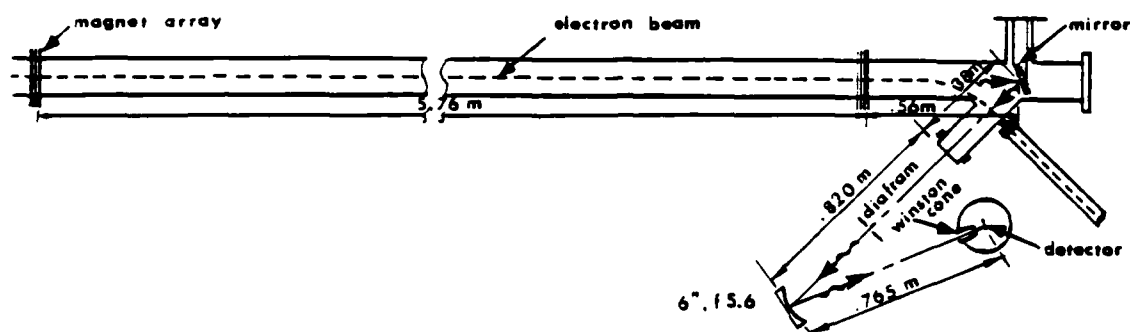


Figure 1. Scheme of the spontaneous radiation layout.

In our experimental design (fig. 1) the source has to be considered an extended source of length L since the detector is not far enough from it. Thus, owing to this, the power collected by the detector would result from the sum of all the elementary powers emitted by the charges $dq = Idx/c$ into the solid angle of the detector $\Delta\Omega^*(x) = A/x^2$. Here A is the area of the collecting lens and x is the distance from the emitting charge. However, since the long beam is emitting inside a cavity, the rays are reflected by its walls (fig. 2) and are guided to the output. Therefore, the far charges are, by this effect, brought nearer to the end of the cavity. In other words the cavity helps to reduce the long source to a point source at a distance $l = h\gamma$ from the output, where h is the dimension of the cavity (fig. 3).

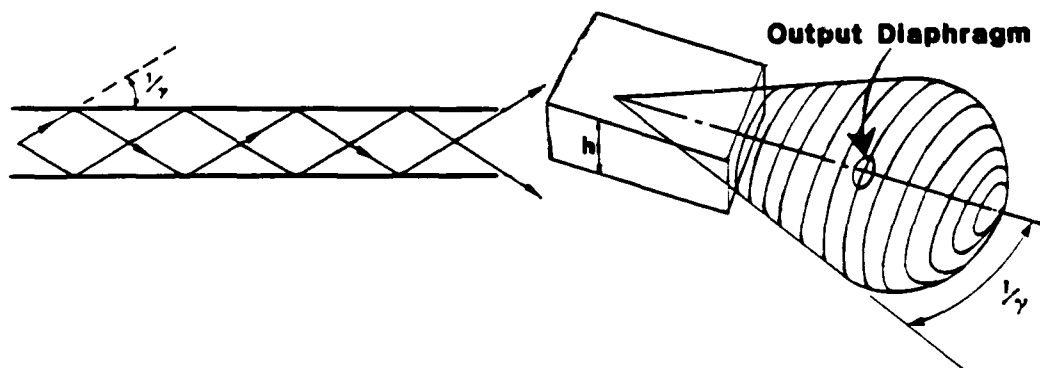


Figure 2. Sketch of two rays trajectories due to the reflections in the cavity.

Figure 3. The border profile of the cavity behaves as an emitting antenna: the angular distribution of the emission pattern is $1/\gamma$.

The area of the collecting lens is $A = 75 \text{ cm}^2$ and its distance to the "apparent" point source is 120 cm. The solid angle subtended at the point source is $\Delta\Omega^* = 6 \cdot 10^{-3}$; the total power going into the aperture is,

$$P_1 = P_{\text{spontaneous}} \frac{\Delta\Omega^*}{\Delta\Omega} \approx 40 \text{ nW}$$

51

The absorption coefficient of quartz is less than 1% per cm and the refractive index $n = 2.1076$ at the wavelength $\lambda = 380 \text{ nm}$. The power P_d is further reduced by the reflectivity R of the 3mm thick crystal quartz window to the value,

$$P_d \approx 10 \text{ nW}$$

52

The radiation is focused on the detector by a concave mirror because any transmitting optics (quartz, silicon, polyethylene, TPX lenses) will have a higher absorption.⁽³⁾ An iris will be used in order to measure a radiation whose bandwidth is determined only by the finite dimension of the wiggler. It will reduce the receiving solid angle to the value $\Delta\Omega = 10^{-4}$ and, in turn, the power P_d to the value

$$P_d \approx 0.5 \text{ nW} \quad (6^1)$$

The linewidth of the radiation is $(\Delta\lambda/\lambda) = (1/2 N) = 0.0031$ and therefore the spectral range is

$$\Delta\nu = 3 \text{ GHz} \quad (7)$$

Spontaneous power measurement

We shall be dealing with very low power so we have to measure it with a calibrated He-cooled Ge-bolometer. This will have a NEP of $1.3 \cdot 10^{-13} \text{ W/Hz}^{1/2}$ with a receiving area of 2 mm.

We have to calculate the effect on the detector's NEP of the background radiation of our layout. It is given by the mean square fluctuation of the thermal source seen by the detector. In our simple case the detector views the radiation in a cone of a half angle α around its normal, the NEP of the detector is⁽⁴⁾

$$\text{NEP}_B = 2 \sqrt{\pi} \sin \alpha \frac{(kT)^{5/2}}{ch^{3/2}} A^{1/2} B_o^{1/2} [J_4(x_1) - J_4(x_2)]^{1/2} \quad (8)$$

where the integrals

$$J_n(x) = \int_0^x \frac{x^n e^{-x}}{(e^x - 1)} dx$$

are tabulated by Rogers and Powell⁽⁵⁾. In (8) T is the temperature of the source, B_o the bandwidth in which the fluctuations are observed, A is the sensitive area of the detector and $x = h\nu/kT$. From (8) observing that: a) the bolometer will be equipped with a cut-on type filter (frequency range $50 \mu\text{m}$ - 3mm), b) $\alpha = \sqrt{\Omega/\pi} = 10^{-1}$ rad and c) a lock-in amplifier will be used (because of the heterodyne receiving the bandwidth is 1 Hz) the NEP results in $\text{NEP}_B = 2 \cdot 10^{-15} \text{ WHz}^{-1/2}$. This does not affect the measurement.

The accuracy of this power measurement can be estimated at about 20%.

Spectral analysis of the spontaneous-FIR radiation

Since the power is very weak, the spectrometer which exploits the heterodyne detection properties would be most suitable. In fact the voltage on the detector is proportional to the powers of the signal P_s and the local oscillator P_{LO} , as well as the cosine of the relative frequency difference, $V = C \sqrt{P_{LO} P_s} \cos[(\omega_s - \omega_{LO})t]$. C is a constant whose value depends on the conversion efficiency. In the far infrared region the critical element of the system is the mixer. The schottky GaAs or InSb diode of the mixer (which combines non-linearly the two radiations) has the basic property of needing high power of radiation from the local oscillator (1-2 mW) in order to have acceptable losses^(4,6). Owing to this, the local oscillator has to be an optically pumped FIR laser⁽⁷⁾ (see fig. 4).

Using the vapor substances mentioned below as active media and a spectrum analyzer with a frequency band of 200 GHz (Tectronix model 492 P) it is possible to cover the FIR spectrum almost entirely. The vapors with good emission lines are: HCOOH (wavelengths $\lambda_{1,2,3} = 393, 420, 433 \mu\text{m}$), CH_3OH ($\lambda_{1,2,3,4} = 42, 70, 97, 119 \mu\text{m}$), CH_2F_2 ($\lambda_{1,2} = 184, 214 \mu\text{m}$), CH_3I ($\lambda = 447 \mu\text{m}$), D_2O ($\lambda = 385 \mu\text{m}$). The cw pump laser CO_2 has to be of a 20 W, single mode, single frequency laser. This sophisticated and expensive local oscillator suggests using a passive instrument as a grating or a Fabry-Perot.

Since it seems to be a good choice to divide the spectrum into 30 lines of width $\Delta\nu = 100 \text{ MHz}$, see fig. 5, the output power would be $P_{\Delta\nu} = 10^{-11} \text{ W}$, the Fabry-Perot only is viable. As a matter of fact the minimum dimension of the grating for the requested resolving power of 10^4 would be 2.5 m . This size, furthermore, would bring about a high background radiation on the detector.

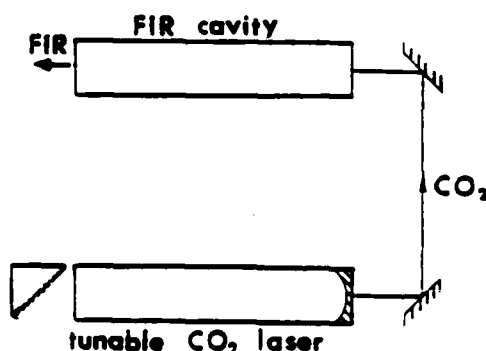


Figure 4. Optically pumped FIR laser system

The Fabry-Perot, with the required resolution of 10^4 , has instead the two surfaces 10 cm apart, as it results from the equation of the resolving power. We have hypothesized for the finesse the value 25-30 which is easily possible.

With the far infrared radiation, the metal meshes are used (fig. 6)⁽¹⁰⁾. The desired values for the reflectivity and losses, $R=0.85$ and $A = 0.03$ respectively, are obtained by choosing the appropriate period g and wire dimensions $2a$ and t of the meshes as shown by the following formulae⁽¹¹⁾

$$R = 1 - \left(\frac{2wg}{\lambda} \right) ; A = \frac{2g}{u} \left(\frac{4\pi \epsilon_0 c}{\lambda_0 g} \right)^{1/2} R \quad (9)$$

where $w = -\text{nsin}(\pi a/g)$, $u = 4a + 2t$ and σ is the conductivity of the wire. Usually the mesh material is Nichel, hence $\sigma = 0.14 \cdot 10^6 \text{ (cm)}^{-1}$. The mesh, which meets the requirements has 400-500 wires/inch and $2a=15.2 \pm 11.2 \text{ } \mu\text{m}$.

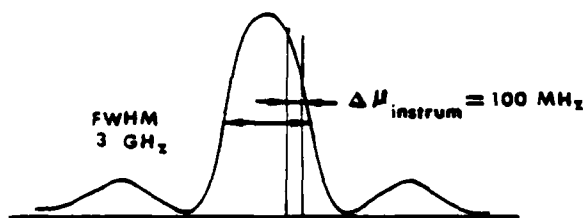


Figure 5. Expected spectrum of the spontaneous emission and bandwidth of the instrument.

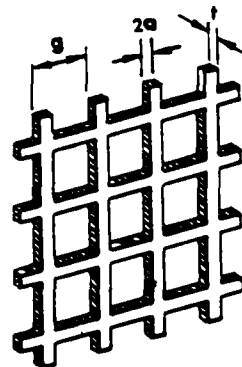


Figure 6. Meshes of the Fabry-Perot interferometer.

The transmitted power is about 65%, that is

$$P \sim 0.6 \cdot 10^{-11} \text{ W} \quad (10)$$

In addition we note that the spectrum can be recorded by tuning either the Fabry-Perot spacing or the electron energy.

Pulse recording

The pulse can be recorded with a Putley detector. This typically has a spectral range of 200-3000 μm and a NEP of $10^{-11} \text{ WHz}^{-1/2}$.

Notes on the laser radiation measurement

With the laser on, the signal is powerful. Consequently it can be recorded with a fast pyroelectric detector; the Molelectron model P3-01 is good.

The power can be measured with a power meter, for instance with the Scientec Inc. power meter model 36-0801.

The spectral analysis has to be more accurate than in the case of spontaneous emission, since the spectrum bandwidth is not limited by the beam length (as in the Stanford experiment), then it can be very narrow.

In the Stanford experiment⁽¹²⁾, the relative spectrum width of the stimulated radiation was $\Delta\nu_{st} = 0.008 \text{ } \mu\text{m}$ unlike $\Delta\nu_{spont} = 0.031 \text{ } \mu\text{m}$ of the spontaneous radiation, and the electron beam length was of some picoseconds. So, with a much longer pulse, the ratio between the two lines could be much less.

Therefore, the heterodyne system seems more useful. As a matter of fact, it may have a resolution of 10^5 .

However, the high level of power in the signal channel allows us to use as a local oscillator a classical millimeter source like a Klystron or an Impatt Diode oscillator of 70 GHz (4mm) or even better 140 GHz. These can be utilized for the generation of higher harmonics by means of a non-linear device, such as a Schottky barrier diode⁽¹³⁾, since they yield enough power. For instance an Impatt Diode of the Hughes Company yields about 50 mW at $\lambda = 2\text{mm}$.

If 70 GHz is the bandwidth of the spectrum analyzer the order n of the needed harmonic is given by

$$\nu_{\text{laser}} - n \nu_{\text{LO}} \approx \frac{70}{2} \text{ GHz}$$

that is, if the frequency of the generator is 140 GHz, the requested harmonic is the sixth. With the conversion efficiency reported in the literature⁽¹⁴⁾, more than 10 μ W could be available. This amount of power is enough to cause the interference with the input signal.

Acknowledgements

We are particularly grateful to J. Kothaus for his useful discussions.

References

1. L.R. Elias, Phys. Rev. Lett. 42 (1979), 15.
2. W.B. Colson, Phys. of Quantum Electronics, Vol 8, pp. 457 (1982) Addison-Wesley.
3. D. Veron, Infrared and Millimeter Waves, K.J. Button Ed. Vol. 2, 1980 (Academic Press).
4. T.G. Blaney, *ibidem*, Vol. 3, p. 2.
5. W.M. Rogers and R.L. Powell, National Bureau of Standards, Circular No. 595 (1958).
6. G.T. Wrixon and W.M. Kelly, Infrared Physics, 18 (1978) 413.
7. D.T. Hodges, Digest Int. Conf. Submm Waves Their Appl. 34d Guildford p. 18 (1978).
8. J. Strong, Concepts of Classical Optics, Freeman, San Francisco, 1958.
9. G.W. Chantry, Submillimeter Spectroscopy, Academic Press, London, N.Y. 1971.
10. K.D. Moller, W.G. Rothschild, Far-Infrared Spectroscopy, Wiley-Interscience, 1971.
11. R. Ulrich, Infrared Phys. 7, (1967) 37.
12. L.R. Elias, W.M. Fairbank, J.M.J. Madey, H.A. Schwettman and T.I. Smith, Phys. Rev. Lett. 36, (1976) 717.
13. E.R. Carlson, M.V. Schneider and T.F. McMaster, IEEE Trans. Microwave Theory Tech MTT-26 (10) (1978) 705.
14. L.C. Robinson, Method of Experimental Physics, L. Marton Ed. Vol. 10, p. 18 (1973), Academic Press.

END

FILMED

386

DTIC